

POWER TO SAVE A LIFE



HealthFirst


HealthFirst

22316 70th Ave. W., #A
Mountlake Terrace, WA 98043

1-800-331-1984

www.healthfirst.com

HEARTSTART ONSITE DEFIBRILLATOR

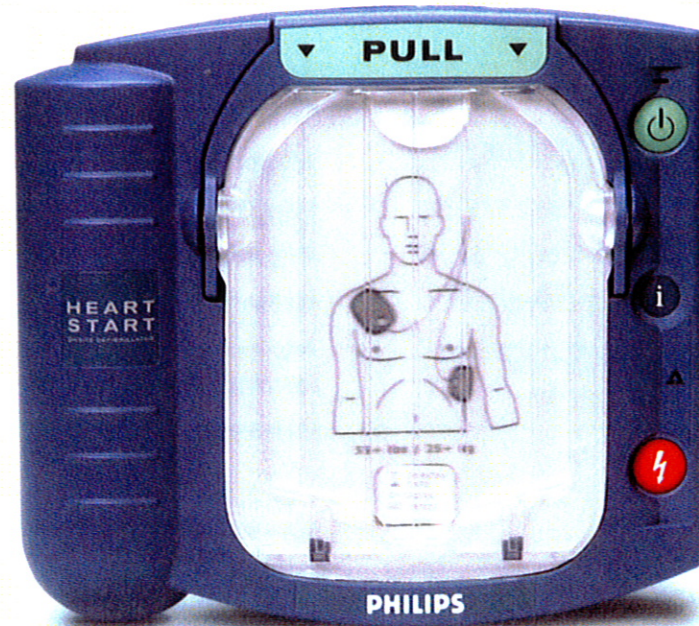

Easy To Use

Using the HeartStart OnSite Defibrillator is simple. Pulling the green handle powers-up the defibrillator and activates voice instructions. These instructions are paced to your actions, to help guide you through the entire process, from placing pads on the patient to delivering a defibrillation shock.


HeartStart OnSite determines if a shock is needed, based on its automated assessment of the victim's heart rhythm:

- ▶ If a shock is needed, the defibrillator directs you to press the flashing orange "Shock" button. Then, HeartStart OnSite delivers a dose of low-energy biphasic therapy, a highly effective defibrillation waveform that is also gentle to the heart.
- ▶ If a shock is not needed, the OnSite Defibrillator instructs you to assess the patient and to perform CPR when necessary. While performing CPR, the defibrillator's voice instructions can be activated to coach you on the frequency and depth of compressions.

HeartStart OnSite also reminds you to call emergency medical services (EMS). And, should EMS need a summary of care, it can be retrieved from the defibrillator's internal memory. An EMS provider simply presses the "i-button" and HeartStart OnSite verbally recounts events from its last clinical use.

Replaceable SMART Pads Cartridges

The cartridge contains two adhesive pads that are peeled and placed on the patient's bare skin as indicated by the pictures on the pads. The pads are "smart" because they can sense that they have been removed from the cartridge and applied to the patient.

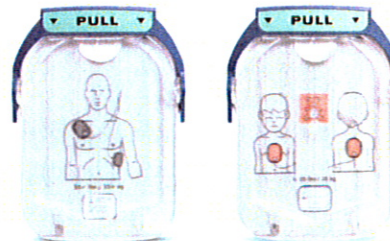

HeartStart OnSite can be used on patients of any age. Special Infant/Child SMART Pads reduce the defibrillator's shock energy, so that you can treat an infant or child suffering sudden cardiac arrest. The Infant/Child Pads cartridge is marked with an indication of the appropriate weight and with a teddy bear icon for ready identification.

To practice your skills, a special training pads cartridge (adult or infant/child) can be installed in the defibrillator. It suspends the defibrillator's ability to shock, while walking you through patient care scenarios.

PHILIPS

TECHNICAL SPECIFICATIONS*

HEARTSTART ONSITE DEFIBRILLATOR

DEFIBRILLATOR

Defibrillator Model	HeartStart M5066A
Defibrillator Family	HS1
How Supplied	Defibrillator, Instructions for Use, battery, adult SMART Pads cartridge (2), Quick Reference
Waveform	Truncated Exponential Biphasic. Waveform parameters adjusted as a function of each patient's impedance.
Energy	Single energy output. Adult: nominal 150 Joules into a 50 ohm load. Infant/Child: nominal 50 Joules into a 50 ohm load. Automatically set based on type of SMART Pads cartridge installed.
Shock-to-Shock Cycle Time	Typically less than 20 seconds.
Protocol	Voice prompts and indicators guide user through protocol. Follows preconfigured settings. Can be modified with HeartStart Event Review software.
Voice Instructions	Detailed voice messages guide responder through use of the defibrillator.
CPR Voice Coaching	Voice instructions in adult and infant/child CPR available at user's option.
Shock Delivery	Via adhesive pads placed on patient's bare skin as illustrated on pads.
Controls	Green SMART Pads cartridge handle, Green On/Off button, Blue i-button, Orange shock button.
Indicators	Ready light; Blue i-button; Caution light.

PHYSICAL

Size	Height	2.8" (7 cm)
	Width	8.3" (21 cm)
	Depth	7.4" (19 cm)
Weight	With battery and pads cartridge	3.3 lbs. (1.5 kg)
	Without battery or pads cartridge	2.4 lbs. (1 kg)

ENVIRONMENTAL/PHYSICAL REQUIREMENTS

Sealing	Drip proof per EN60529 class IPX1. Solid Objects per EN60529 class IP2X.
Temperature	Operating: 32° - 122° F (0° - 50° C) Standby: 50° - 109° F (10° - 43° C)
Humidity	Operating: 0% to 95% relative, non-condensing Standby: 0% to 75% relative, non-condensing
Altitude	Operating: 0 to 15,000 feet Standby: 0 to 8,500 feet >48 hours and 8,500 to 15,000 feet <48 hours
Shock/Drop Abuse	Withstands 1 meter drop to any edge, corner or surface.
Vibration	Meets EN1789 random and swept sine, road ambulance specification in operating and standby states.
EMI (Radiated/Immunity)	Meets EN55011 Group 1 Level B Class B and EN61000-4-3.

PATIENT ANALYSIS SYSTEM

Patient Analysis	Evaluates patient ECG and signal quality to determine if a shock is appropriate, and evaluates connection impedance for proper defibrillation pad contact.
Sensitivity/Specificity	Meets AAMI DF39 guidelines and AHA recommendations for adult defibrillation (Circulation 1997;95:1677-1682).
Artifact Detection	The effects of pacemaker artifact and electrical noise are minimized with artifact detection.

BATTERY (M5070A)

Type	9 Volt DC, 4.2 Ah, lithium manganese dioxide, disposable long-life primary cell.
Capacity	Minimum 90 shocks or 3 hours of operating time.
Install-By Date	Battery is labeled with an install-by date of at least five years from date of manufacture.
Standby Life	Four years typical when battery is installed by the install-by date. (Will power the AED in standby state within the specified standby temperature range, assuming one battery insertion test and no defibrillation uses.)

SMART PADS

Adult SMART Pads Cartridge	M5071A defibrillation pads for patients 8 years of age and older or 55 lbs. (25 kg) and over.
Infant/Child SMART Pads Cartridge	M5072A defibrillation pads for patients under 8 years of age or 55 lbs. (25 kg).
Energy Delivered	Adult: nominal 150 Joules into a 50 ohm load. Infant/Child: nominal 50 Joules into a 50 ohm load.
How Supplied	Disposable cartridge, containing adhesive defibrillation pads, clicks into defibrillator for an integrated pads solution.
Active Surface Area	13.2 in 2 (85 cm 2) each
Cable Length	Adult pads: 54 inch (137.1 cm) Infant/Child pads: 40 inch (101.6 cm)
Use-By Date	Cartridge is labeled with a use-by date of at least two years from date of manufacture.

TRAINING PADS

Adult Training Pads Cartridge	M5073A
Infant/Child Training Pads Cartridge	M5074A
Function	Special pads place HeartStart OnSite into training mode and disable its energy delivery capability. Feature 8 real-world training scripts.

AUTOMATED AND USER-ACTIVATED SELF-TESTS

Daily Automatic Self-tests	Tests internal circuitry, waveform delivery system, pads cartridge and battery capacity.
Pads Integrity Test	Specifically tests readiness-for-use of pads (gel moisture).
Battery Insertion Test	Upon battery insertion, extensive automatic self-tests and user-interactive test check device readiness.
Status Indicator	Blinking green Ready light indicates ready for use.

DATA RECORDING AND TRANSMISSION

Infrared	Wireless transmission of event data to personal computer using the IrDA protocol.
HeartStart Event Review Software	Data management software (optional) for download and review of data retrieved through defibrillator's infrared data port.
Data Stored	First 15 minutes of ECG and the entire incident's events and analysis decisions.

* Refer to HeartStart OnSite Defibrillator Instructions for Use for detailed product instructions.

All specifications based on 25° C unless otherwise noted. The defibrillator and its accessories are made of latex-free materials.



HealthFirst

HealthFirst Corp.
22316 70th Ave. W., #A
Mountlake Terrace, WA 98043
1-800-331-1984
www.healthfirst.com